

**INTENDED USE**

This human coagulation Factor XI antigen assay is intended for the quantitative determination of total Factor XI antigen in human plasma and serum. **For research use only.**

**BACKGROUND**

Factor XI is a disulfide linked two-chain glycoprotein zymogen and is the precursor of the coagulation enzyme Factor XIa [1]. Factor XI consists of two identical monomers and circulates in plasma in complex with kininogen [2]. Factor XI is activated by Factor XIIa and converts Factor IX to Factor IXa during the intrinsic pathway of the coagulation cascade [3].

**ASSAY PRINCIPLE**

Human Factor XI will bind to the capture antibody coated on the microtiter plate. Both Factor XI and XIa will react with the antibody on the plate. After appropriate washing steps, biotinylated primary antibody binds to the captured protein. Excess primary antibody is washed away, and bound antibody is reacted with horseradish peroxidase conjugated streptavidin. TMB substrate is used for color development at 450nm. A standard calibration curve is prepared along with the samples to be measured using dilutions of human Factor XI. Color development is proportional to the concentration of Factor XI in the samples.

**STANDARD CALIBRATION**

Factor XI standard provided is calibrated against the WHO 2nd International Standard for Factor XI, Plasma, Human distributed by NIBSC (15/180), South Mimms, Potters Bar, Hertfordshire, UK. **See C of A for lot specific Calibration of Standard.**

**REAGENTS PROVIDED**

- **96-well antibody coated microtiter strip plate** (removable wells 8x12) containing anti-human Factor XI antibody, blocked and dried.
- **10X Wash buffer:** 1 bottle of 50ml
- **Human Factor XI standard:** 1 vial lyophilized standard
- **Anti-human Factor XI primary antibody:** 1 vial lyophilized polyclonal antibody
- **Horseradish peroxidase-conjugated streptavidin:** 1 vial concentrated HRP labeled streptavidin
- **TMB substrate solution:** 1 bottle of 10ml solution

**STORAGE AND STABILITY**

Store all kit components at 4°C upon arrival. Return any unused microplate strips to the plate pouch with desiccant. Reconstituted standard and primary may be stored at -80°C for later use. Do not freeze-thaw the standard and primary antibody more than once. Store all other unused kit components at 4°C. This kit should not be used beyond the expiration date.

**OTHER REAGENTS AND SUPPLIES REQUIRED**

- Microtiter plate shaker capable of 300 rpm uniform horizontally circular movement
- Manifold dispenser/aspirator or automated microplate washer
- Microplate reader capable of measuring absorbance at 450 nm
- Pipettes and Pipette tips
- Deionized or distilled water
- Polypropylene tubes for dilution of standard
- Paper towels or laboratory wipes
- 1N H<sub>2</sub>SO<sub>4</sub> or 1N HCl
- Bovine Serum Albumin Fraction V (BSA)
- Tris(hydroxymethyl)aminomethane (Tris)
- Sodium Chloride (NaCl)

## PRECAUTIONS

- FOR LABORATORY RESEARCH USE ONLY. NOT FOR DIAGNOSTIC USE.
- Do not mix any reagents or components of this kit with any reagents or components of any other kit. This kit is designed to work properly as provided.
- Always pour peroxidase substrate out of the bottle into a clean test tube. Do not pipette out of the bottle as contamination could result.
- Keep plate covered except when adding reagents, washing, or reading.
- DO NOT pipette reagents by mouth and avoid contact of reagents and specimens with skin.
- DO NOT smoke, drink, or eat in areas where specimens or reagents are being handled.

## PREPARATION OF REAGENTS

- **TBS buffer:** 0.1M Tris, 0.15M NaCl, pH 7.4
- **Blocking buffer (BB):** 3% BSA (w/v) in TBS
- **1X Wash buffer:** Dilute 50ml of 10X wash buffer concentrate with 450ml of deionized water

## SAMPLE COLLECTION

Collect plasma using EDTA or citrate as an anticoagulant. Centrifuge for 15 minutes at 1000xg within 30 minutes of collection. Assay immediately or aliquot and store at  $\leq -20^{\circ}\text{C}$ . Avoid repeated freeze-thaw cycles.

## ASSAY PROCEDURE

Perform assay at room temperature. Vigorously shake plate (300rpm) at each step of the assay.

### Preparation of Standard

**Reconstitute standard according to the C of A.** Agitate gently to completely dissolve contents.

Dilution table for preparation of human Factor XI standard:

Factor XI concentration (ng/ml)	Dilutions
10	900 $\mu\text{l}$ (BB) + 100 $\mu\text{l}$ (from vial)
5	500 $\mu\text{l}$ (BB) + 500 $\mu\text{l}$ (10ng/ml)
2.5	500 $\mu\text{l}$ (BB) + 500 $\mu\text{l}$ (5ng/ml)
1	600 $\mu\text{l}$ (BB) + 400 $\mu\text{l}$ (2.5ng/ml)
0.5	500 $\mu\text{l}$ (BB) + 500 $\mu\text{l}$ (1ng/ml)
0.25	500 $\mu\text{l}$ (BB) + 500 $\mu\text{l}$ (0.5ng/ml)
0.1	600 $\mu\text{l}$ (BB) + 400 $\mu\text{l}$ (0.25ng/ml)
0.05	500 $\mu\text{l}$ (BB) + 500 $\mu\text{l}$ (0.1ng/ml)
0.02	600 $\mu\text{l}$ (BB) + 400 $\mu\text{l}$ (0.05ng/ml)
0.01	500 $\mu\text{l}$ (BB) + 500 $\mu\text{l}$ (0.02ng/ml)
0	500 $\mu\text{l}$ (BB) Zero point to determine background

**NOTE: DILUTIONS FOR THE STANDARD CURVE AND ZERO STANDARD MUST BE MADE AND APPLIED TO THE PLATE IMMEDIATELY.**

### Standard and Unknown Addition

Remove microtiter plate from bag and add 100 $\mu\text{l}$  Factor XI standards (in duplicate) and unknowns to wells. Carefully record the position of standards and unknowns. Shake plate at 300rpm for 30 minutes. Wash wells three times with 300 $\mu\text{l}$  wash buffer. Remove excess wash by gently tapping plate on paper towel or kimwipe.

**NOTE:** The assay measures total human Factor XI in the 0.01-10 ng/ml range. Samples giving human Factor XI levels above 10ng/ml should be diluted in blocking buffer before use. A 1:2,000-1:10,000 dilution for normal human plasma is suggested for best results.

### Primary Antibody Addition

Reconstitute primary antibody by adding 10ml of blocking buffer directly to the vial and agitate gently to completely dissolve contents. Add 100 $\mu\text{l}$  to all wells. Shake plate at 300rpm for 30 minutes. Wash wells three times with 300 $\mu\text{l}$  wash buffer. Remove excess wash by gently tapping plate on paper towel or kimwipe.

## **Streptavidin-HRP Addition**

Briefly centrifuge vial before opening. **See C of A for lot specific dilution instructions.** Add 100 $\mu$ l of your dilution to all wells. Shake plate at 300rpm for 30 minutes. Wash wells three times with 300 $\mu$ l wash buffer. Remove excess wash by gently tapping plate on paper towel or kimwipe.

## **Substrate Incubation**

Add 100 $\mu$ l TMB substrate to all wells and shake plate for 3-10 minutes. Substrate will change from colorless to different strengths of blue. Quench reaction by adding 50 $\mu$ l of 1N H<sub>2</sub>SO<sub>4</sub> or HCl stop solution to all wells when samples are visually in the same range as the standards. Add stop solution to wells in the same order as substrate upon which color will change from blue to yellow. Mix thoroughly by gently shaking the plate.



## **Measurement**

Set the absorbance at 450nm in a microtiter plate spectrophotometer. Measure the absorbance in all wells at 450nm. Subtract zero point from all standards and unknowns to determine corrected absorbance (A<sub>450</sub>).

## **Calculation of Results**

Plot A<sub>450</sub> against the amount of Factor XI in the standards. Fit a straight line through the linear points of the standard curve using a linear fit procedure if unknowns appear on the linear portion of the standard curve. Alternatively, create a standard curve by analyzing the data using a software program capable of generating a four-parameter logistic (4PL) curve fit. The amount of Factor XI in the unknowns can be determined from this curve. If samples have been diluted, the calculated concentration must be multiplied by the dilution factor.

A typical standard curve (EXAMPLE ONLY):

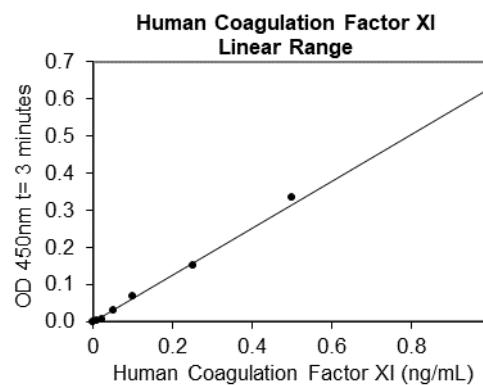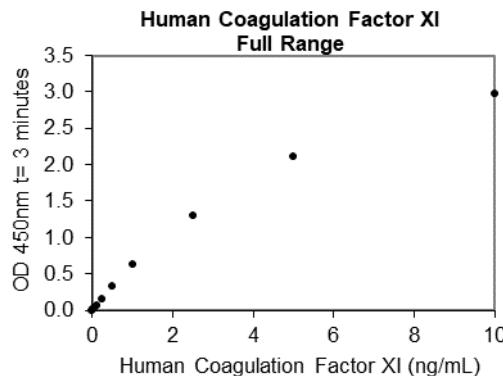

## **EXPECTED VALUES**

The concentration of Factor XI in normal human plasma ranges from 3.0 to 6.0  $\mu$ g/ml [4].

## **PERFORMANCE CHARACTERISTICS**

**Sensitivity:** The minimum detectable dose (MDD) was determined by adding two standard deviations to the mean optical density value of twenty zero standard replicates and calculating the corresponding concentration. **See C of A for lot specifications.**

**Intra-assay Precision:** Three samples of known concentration were tested twenty times on one plate to assess intra-assay precision.

Sample	1	2	3
n	20	20	20
Mean (ng/ml)	0.045	3.26	5.8
Standard Deviation	0.004	0.066	0.216
CV (%)	9.42	2.04	3.70

**Inter-assay Precision:** Three samples of known concentration were tested in ten independent assays to assess inter-assay precision.

Sample	1	2	3
n	10	10	10
Mean (ng/ml)	0.031	0.315	3.12
Standard Deviation	0.002	0.017	0.12
CV (%)	7.55	5.28	3.86

**Recovery:** The recovery of antigen spiked to levels throughout the range of the assay in blocking buffer was evaluated.

Sample	1	2	3	4
n	4	4	4	4
Mean (ng/ml)	0.04	0.13	0.66	7.08
Average % Recovery	96	102	94	101
Range	89-107%	97-111%	91-97%	94-104%

**Linearity:** To assess the linearity of the assay, human plasma samples containing high concentrations of antigen were serially diluted to produce samples with values within the dynamic range of the assay.

Sample	1:2	1:4	1:8	1:16
n	4	4	4	4
Average % of expected	102	105	105	98
Range	96-108%	97-108%	97-118%	90-116%

**Specificity:** This assay recognizes natural and recombinant human FXI. Significant cross reaction is observed with pooled normal plasma from porcine serum, cyno and rhesus monkey. Pooled normal plasma from mouse, pig, rabbit, dog, and sheep were assayed for cross-reactivity. No significant cross-reactivity was observed.

#### Example of ELISA Plate Layout

96 Well Plate: 22 Standard wells, 74 Sample wells

	1	2	3	4	5	6	7	8	9	10	11	12
A	0	0.01 ng/ml	0.02 ng/ml	0.05 ng/ml	0.1 ng/ml	0.25 ng/ml	0.5 ng/ml	1 ng/ml	2.5 ng/ml	5 ng/ml	10 ng/ml	
B	0	0.01 ng/ml	0.02 ng/ml	0.05 ng/ml	0.1 ng/ml	0.25 ng/ml	0.5 ng/ml	1 ng/ml	2.5 ng/ml	5 ng/ml	10 ng/ml	
C												
D												
E												
F												
G												
H												

**Sample Values:** Samples were evaluated for the presence of the antigen at varying dilutions.

Sample Type	Dilution	Mean (μg/ml)
Citrate Plasma	1:5,000	2.72
	1:10,000	2.79
EDTA Plasma	1:5,000	3.17
	1:10,000	3.48
Heparin Plasma	1:5,000	3.1
	1:10,000	3.43
Serum	1:5,000	4.14
	1:10,000	4.4

#### DISCLAIMER

This information is believed to be correct but does not claim to be all-inclusive and should be used only as a guide. The supplier of this kit shall not be held liable for any damage resulting from handling of or contact with the above product.

#### REFERENCES

1. Kurachi K and Davie EW.: Methods in Enzymology. 1981, 80:211-220.
2. Thompson RE, et al.: J Clin Invest. 1977, 60:1376.
3. Walsh PN, et al.: Methods in Enzymology. 1993, 222:65-96.
4. Bouma BN, et al.: Blood. 1983, 62:1123-1131.